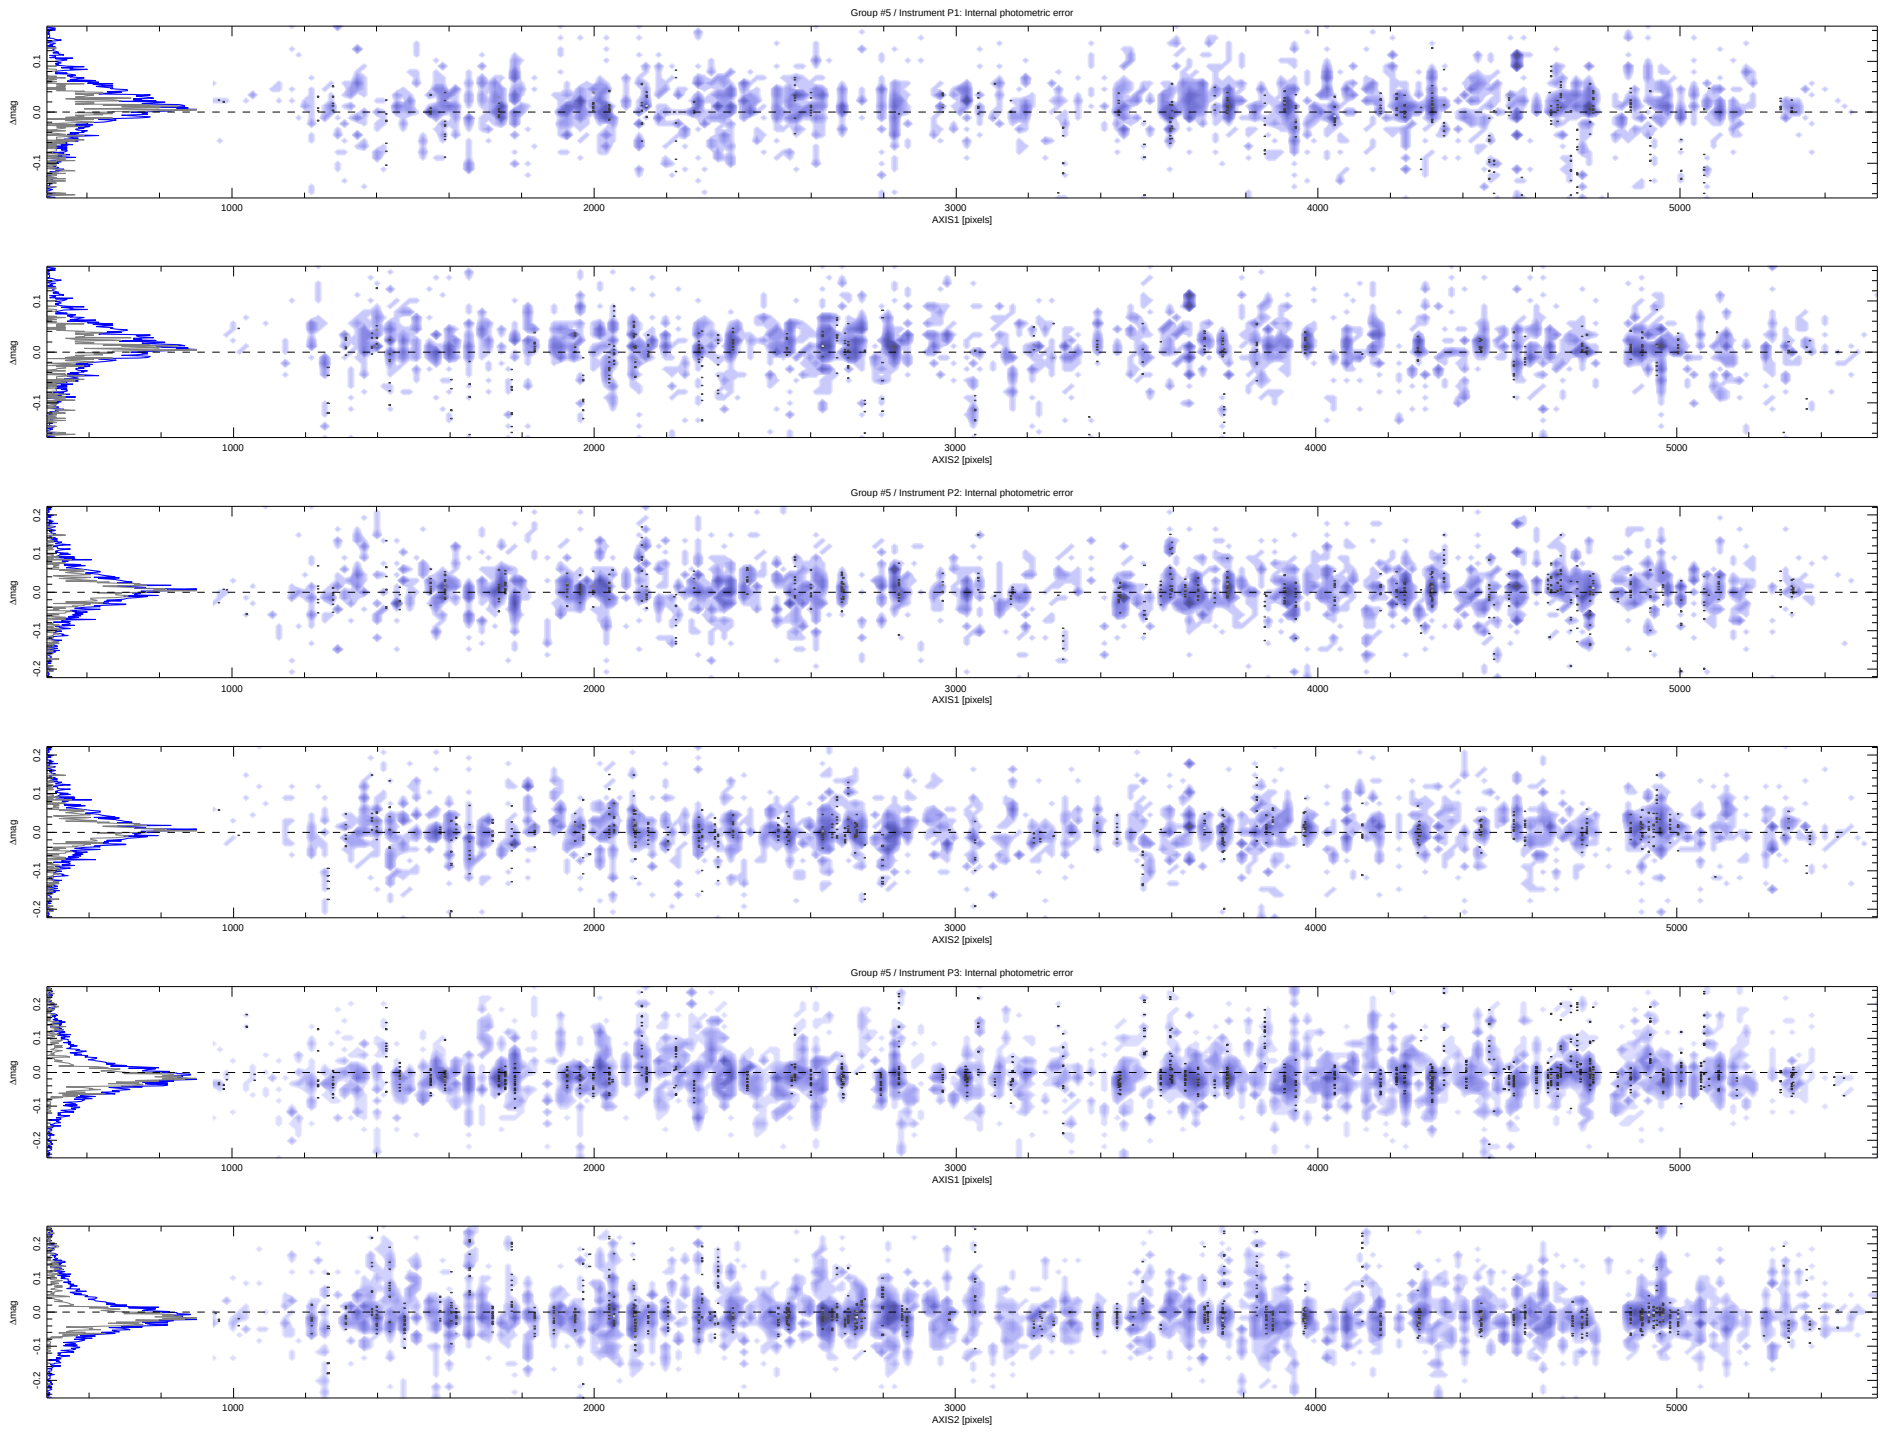
Group #5 / Instrument P1: Internal photometric error
Δmag
AXIS1 [pixels]
AXIS2 [pixels]
Group #5 / Instrument P2: Internal photometric error
Group #5 / Instrument P3: Internal photometric error

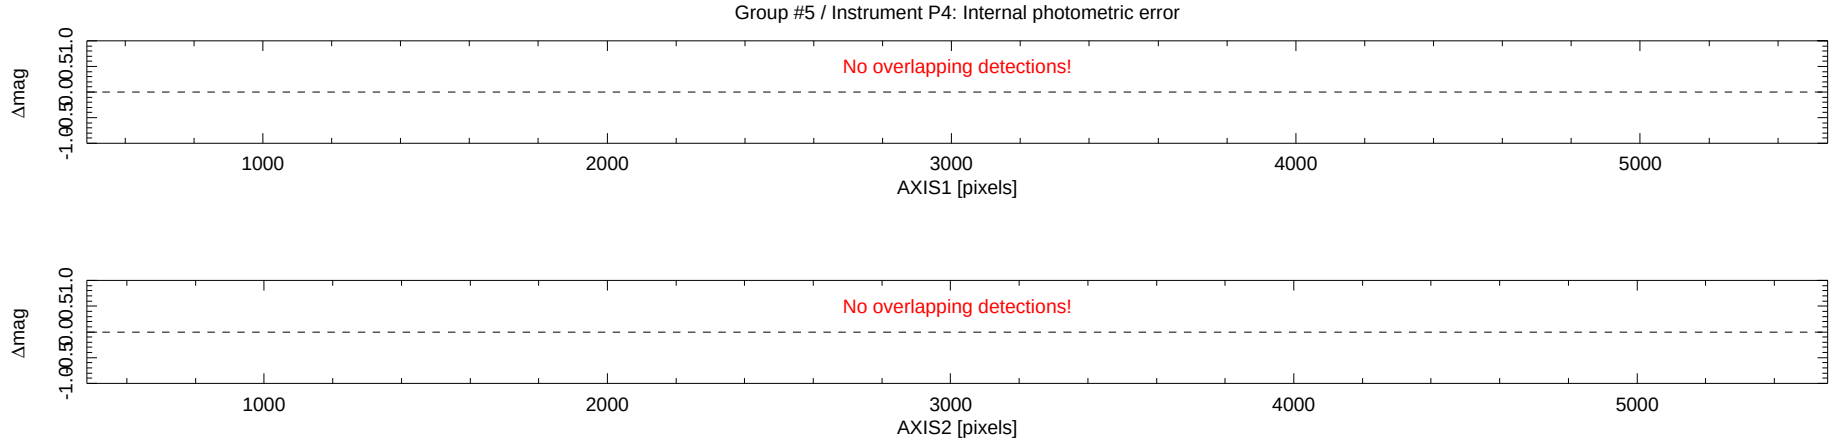
Group #5 / Instrument P4: Internal photometric error
Δmag
-1.0
-0.5
0.0
0.5
1.0
No overlapping detections!
1000
2000
3000
4000
5000
AXIS1 [pixels]

Δmag
-1.0
-0.5
0.0
0.5
1.0
No overlapping detections!
1000
2000
3000
4000
5000
AXIS2 [pixels]